

---

# Critical Review of Burn Depth Assessment Techniques: Part II. Review of Laser Doppler Technology

---

Amín D. Jaskille, MD,\*† Jessica C. Ramella-Roman, PhD,‡ Jeffrey W. Shupp, MD,\*†  
Marion H. Jordan, MD,\*† James C. Jeng, MD\*†

The judgment of which wounds are expected to heal within 21 days is one of the most difficult and important tasks of the burn surgeon. The quoted accuracy of 64 to 76% by senior burn surgeons underscores the importance of an adjunct technology to help make this determination. A plethora of techniques have been developed in the last 70 years. Laser Doppler imaging (LDI) is one of the most recent and widely studied of these techniques. The technology provides an estimate of perfusion through the burn wound, the assumption being that a lower perfusion correlates with a deeper wound and, therefore, a longer time to heal. Although some reports suggest accuracy between 96 and 100% and that it does this 2 days ahead of clinical judgment, others have questioned its applicability to clinical practice. This article, the second of a two-part series, has two objectives: 1) a review of the Doppler principle and how the LDI uses it to estimate perfusion; and 2) a critical assessment of the burn literature on the LDI. Part I provides a historical perspective of the different technologies used through the last 70 years to assist in the determination of burn depth. Laser Doppler has brought technology closer to provide a reliable adjuvant to the clinical prediction of healing, yet, caution is warranted. A clear understanding of the limitations of LDI is needed to put the current research in perspective to find the right clinical application for LDI. (*J Burn Care Res* 2010;31:151–157)

The judgment of burn depth is of paramount clinical importance, because it helps in the determination of whether a burn wound is expected to heal on its own within 3 weeks, or whether excision and grafting is necessary. The most common way of assigning depth is by clinical examination, according to the wound appearance<sup>1–3</sup> and its response with the pinprick test.<sup>4</sup> Despite assessing for these clinical signs, even in experienced hands, the best clinical estimates are only 64 to 76% accurate,<sup>5,6</sup> which translates into either a delay in treatment or unnecessary surgery. A wide variety of modalities have been developed to aid in the determination of burn wound depth and to help pre-

dict a burn wound's potential for healing, and these have been discussed elsewhere.<sup>7</sup> One of the most recent, and widely studied, of these technologies is laser Doppler imaging (LDI). Initially described by Stern<sup>8</sup> in 1975 as a point-contact technology, allowing the study of a 1-mm<sup>2</sup> area only, modifications during the 1990s permit noncontact scanning from a distance up to 1.6 meters away, allowing for an area 500 mm × 700 mm to be scanned in about 6 minutes.<sup>9</sup> To avoid confusion, the point-contact technology initially described by Stern will be termed LD flowmetry and the currently used, noncontact distance scanner described by Niazi et al<sup>9</sup> LD scanning. This review is focused on LD scanning, because this is probably the most commonly used modality today. LD flowmetry will be referenced for historical purposes.

LD scanning is one of the most recent and most tested adjuvants to determine burn depth. Its quoted accuracy in predicting that which wounds are not expected to heal within 3 weeks is between 96 and 100%,<sup>10–13</sup> and it does this in advance of clinical judgment by a median of 2 days.<sup>14</sup> It is noninvasive, relatively fast, and seemingly simple to use. The question

*From the \*The Burn Center, Department of Surgery, Washington Hospital Center, Washington, DC; †MedStar Research Institute, Washington, DC; and ‡Department of Biomedical Engineering, The Catholic University of America, Washington, DC.*

*Address correspondence to James C. Jeng, MD, The Burn Center at Washington Hospital Center, 110 Irving Street, NW, Suite 3B-55, Washington, DC, 20010.*

*Copyright © 2010 by the American Burn Association. 1559-047X/2010*

*DOI: 10.1097/BCR.0b013e3181c7ed60*

arises why has this technology not gained more widespread use? Some have questioned the validity of the findings in relation to the clinical practice of burns, leading to the conclusion that the technology is best suited as a research tool and not yet ready for clinical practice.<sup>15</sup> Part I of this two-part series provided a historical review of the other techniques used in the last 70 years, thus providing a framework for this study. The purpose of this article is to explain LD technology, to understand what it is capable of and what its limitations are, and then, to critically review the current burn literature.

### Laser Doppler Technology

The Doppler effect is a change of frequency in an impinging waveform induced by a moving object. In LD, laser light at a singular frequency  $f$  strikes a moving object and it is scattered into a new direction at a different frequency  $f'$ . The relationship between incident and reflected light is shown in Eq. (1), where  $v$  is the relative velocity of the moving object and  $c$  is the speed of light.

$$f' - f = \Delta f = \frac{2v}{c - v}f \quad (1)$$

The factor of 2 in this equation is because of the motion of the object relatively to both the source and the detector; if the moving object was also the source of the wave, then this factor would not be necessary. It is also important to note that only the component of the velocity vector directed toward or away from the detector contributes to the Doppler frequency.

Because the velocity of the laser light is much larger than the object's velocity,  $c \gg v$ , then Eq. (1) can be simplified to the following expression:

$$\Delta f = \frac{v}{c}f \quad (2)$$

By substituting the relationship between source wavelength  $\lambda$  and speed of light  $c = \lambda f$  in Eq. (2), we obtain the relationship between object velocity and frequency change, also known as Doppler shift, as follows:

$$v = \frac{\lambda}{2}\Delta f \quad (3)$$

Finally, let us consider a practical situation where the laser beam impinges on a red blood cell at an angle  $\phi$  to the normal of the direction of the moving flow. Its scattered component is then collected at a different angle, giving us a general equation of the form:

$$v = \frac{\lambda}{2\sin(\phi)\cos(\theta)}\Delta f \quad (4)$$

Equations (1)–(4) describe the Doppler principle for a single moving object where  $\theta$  is the angle between the direction of motion and the bisector of the angle determined by the incident beam direction and the collection direction. This is not the case when dealing with skin perfusion where superficial vasculature is a mixture of different sizes of capillaries, arterioles, and venules, as well as different red blood cell velocities. The result is a spread of Doppler-shifted frequencies about an average value and the generation of a homodyne signal generally used to investigate Brownian motion, as well as a heterodyne signal caused by the moving blood.<sup>16</sup>

The quantity of perfusion obtained through a typical LD can be defined as the product of the magnitude of the velocity vector and the concentration of moving blood cells in the probed area. This depends on the tissue optical properties and the used wavelength. The fact that the probing depth changes for different tissues and different individuals is one of the major drawbacks in LD and contributes to the lack of absolute units for this technique. Light penetration depth, and consequently flow-probing depth, depends on the source wavelength. In the skin, short visible wavelengths have a shallower penetration than longer near-infrared wavelengths. Typical penetration values are between 1 and 2 mm. Some work is being conducted using multiple wavelengths<sup>17,18</sup> and probes with several fibers appropriately spaced,<sup>19</sup> but much work remains to be performed to standardize this technique.

An important concept when using LD to assess perfusion is the "biological zero." This refers to the signal that remains in an area following vascular occlusion with a cuff to a suprasystolic pressure.<sup>20</sup> Despite the fact that the main source of the signal has been eliminated, a spurious continuous signal remains. There are several possible sources for this persistent signal, among them: 1) collateral circulation through bone, 2) fluid and cellular movement within the interstitium, 3) movement within the intravascular compartment that is unrelated to flow (ie, red cell aggregation), 4) residual vasomotion, and 5) Brownian motion of macromolecules.<sup>21</sup> Although a clear understanding of the biological zero is still lacking, and there is debate on how to best approximate it mathematically,<sup>22,23</sup> there is evidence that it changes with edema formation in vivo<sup>24</sup> and in skin hyperthermic conditions.<sup>25</sup> Understanding that there are many conditions that may alter the biological zero, some have suggested that it should be measured under ev-

ery experimental/clinical condition and subtracted from the flow signal.<sup>21</sup>

LDI uses the Doppler principle for generating images of flow and perfusion in a dynamic biological media. Different from the more common fiber-based systems (ie, LD flowmetry as described by Stern<sup>8</sup>), LDI systems do not need contact with the skin. This is a great advantage when dealing with lesions such as those seen after thermal injury where pain and risk on infection from probe contact are important considerations.

Two types of LDI are commercially available. One type of LDI uses a scanning laser point source across a region of interest and a silicon detector to capture the Doppler shift at different points in the skin. This type of system is able to generate images of an area up to 500 mm × 500 mm in few minutes (reported values are up to 6 minutes). A typical instrumentation layout for a LDI system is shown in the Figure 1.<sup>16,26</sup>

This system consists of a laser source (Helium Neon lasers or laser diodes at 633 and 780 nm are typical), a detection assembly (silicon photodiodes and lenses) connected to a Doppler signal processing system, and a scanning mirror. The mirror is connected to a galvanometer-based scanner (or other motorized scanning system), and its function is to redirect the source laser light into a desired pattern and area (Figure 1). Another function of the mirror is to redirect the light backscattered from the skin toward the lenses and finally to the photodiodes. The mirror's motion is computer controlled.

This technique is similar to its fiber-based counterpart in the sense that the Doppler shift is observed in one point at a time. Several of these points are assembled to create an image. The drawback is that when the laser is scanning, any movement of the object will result in image artifacts. A technique based on snapshot imaging is hence preferable.

The second type of LDI system uses the fluctuation of speckle patterns on the skin as a contrast mechanism for blood perfusion. This type of imaging is often called speckle contrast imaging. Speckle con-

trast imaging produces images of superficial vasculature average blood flow.

A typical speckle-based LDI system layout is shown in Figure 2. It consists of a laser source and a computer-controlled camera. When laser light hits the skin, a speckle pattern is formed at the detector because of the coherence of the source and the microstructure of the skin. The speckle moves because of blood and tissue movements. The contrast is determined by the standard variation of the intensity fluctuation to the mean intensity.<sup>16</sup> Any type of movement will cause averaging of the speckle pattern, a characteristic that is both useful when determining perfusion and problematic because dealing with live subjects. Important parameters in speckle-contrast LDI are the exposure time, which needs to be in the order of the correlation time of the speckle, and the pixels/speckle ratio. Too few pixels per speckle will result in reduced accuracy, whereas too many pixels per speckle will cause low spatial resolution. A number between five and seven pixels per speckle has shown to produce reliable results.<sup>27</sup>

### Burn Literature

In his original description of the LD technology, Stern<sup>8</sup> cautioned about some of its limitations. He stated that the measurements were very labile and being affected by the room's temperature, the patient's position, respiratory rate, and even emotional stimulation. Some of these findings have been echoed by others more recently.

By using LD flowmetry, Waxman et al studied the effect of wound temperature on the readings obtained. He scanned unhealed burn wounds and found that at a lower temperature (35°C), specificity was

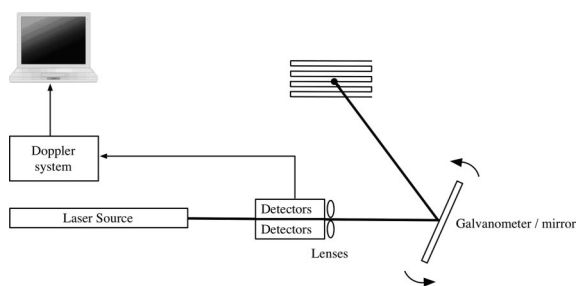


Figure 1. Laser Doppler scanning imager.

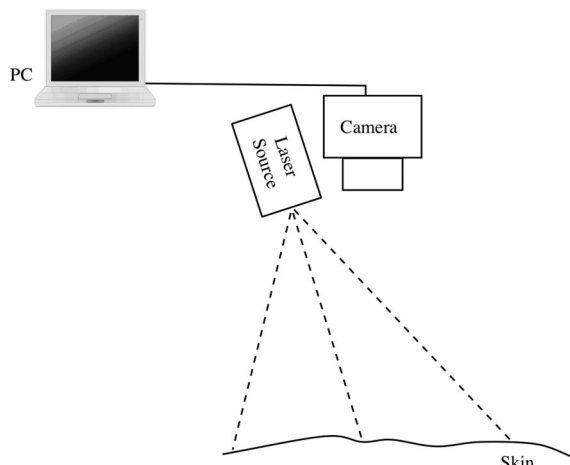


Figure 2. Layout of a speckle-based laser Doppler imaging system.

very high (100%) but there was a poor sensitivity; however, at a temperature of 44°C sensitivity improved to 93%, but specificity decreased.<sup>28</sup> Barachini et al assessed perfusion in healed burn wounds (wounds had healed either with skin grafts or on their own) and found that they behaved differently than open wounds. He found no difference in the perfusion units (PU) when changing the skin temperature between 36°C and 41°C.<sup>29</sup> Both of these studies were performed with LD flowmetry. Different researchers working with LD scanning have maintained the room temperature between 22°C and 25°C,<sup>11,12</sup> but the actual wound temperature is not detailed in these studies. A study assessing the effect of wound temperature on PU using LD scanning is lacking.

One of the advantages that LD scanning has over the older LD flowmetry is the fact that the wound can be assessed at from distance. This is more comfortable for the patient who suffers less pain, allows for the study of a larger area, and, in theory, should help limit wound infection rate as there is no contact with the tissue. This brings several questions. First, which is the ideal distance from the wound? In their original description, Niazi et al<sup>9</sup> scanned from a distance of 1.6 meters. Other researchers have used 20 cm,<sup>10</sup> 50 cm,<sup>14</sup> variable distances of 30 to 40 cm,<sup>30</sup> or 40 to 70 cm,<sup>12</sup> whereas, in other reports, the distance was not documented.<sup>11</sup> Often, as is the case with research, the results of one study were used as the basis for the next study. If there is no consistent distance from which to scan, the question that arises is what is the effect of changing this distance?

In an initial study assessing the effect of increasing the distance between target and scanner, it was found that this increased the PU.<sup>31</sup> A follow-up report, using a different brand of LD,<sup>9</sup> however, found the opposite, increasing the distance decreased the PU.<sup>32</sup> The difference could be attributed to different equipment using different ways of “normalizing” the perfusion signal; however, this raises concern as it makes results from one study difficult to reproduce, let alone apply to clinical practice.

Another question that comes up when scanning from a distance is what is the effect of changing the scanning angle, or more practical, what is the effect of scanning over a curvilinear surface. Two studies have looked at this and found a decrease of up to 50% in perfusion when scanning over curvilinear surfaces, attributed simply to the curvature and not a true decrease in perfusion.<sup>32,33</sup>

There are wound-specific factors that have been found to play a role in the readings obtained, for example, the “wetness” of the wound decreases PU between 13 and 33%.<sup>32</sup> In an attempt to limit the

time that a wound is uncovered and open to air, some researchers have scanned through a transparent dressing. Holland et al assessed the effect of the burn wound dressing on the LD scanning readings, particularly if different clear, or transparent, dressings would have an effect when scanning through them, rather than having to remove them. For their study, they used a healthy volunteer whose arm was subjected to pressure for 2 minutes. They found that different types of dressing and different ways of applying them affected the output measurement.<sup>34</sup>

The questions about the effect of temperature, distance, angle, wound dressing, and dryness/wetness in the wound are all methodological questions that can, and should, be standardized to improve the power and applicability of the work being conducted. A more basic question is what information does the LD scanner telling us? The answer, at its root, is simple; it tells us how much movement there is in the skin (the product of average blood cell speed and concentration of moving blood cells). This has been equated with perfusion under the assumption that in the absence of movement because of respiration or shivering, the only moving particles in the area in question are blood cells.<sup>11</sup> although at first glance, and under certain conditions, this statement might be true, this is often not the case with burn wounds.

A burn wound is a very dynamic environment, particularly in the first 24 to 48 hours. There is initially an inflammatory reaction, which is characterized, among other things, by a hyperemic response and by the formation of edema. Edema is formed by fluid particles moving out of the capillaries and into the interstitium. Similarly, at some point, this edema fluid will be reabsorbed into the capillaries and lymphatics, representing more movement of particles. Although the set “biological zero” can accommodate for some of this fluid-shift phenomenon, the effect in the recorded PU is in question. Furthermore, the biological zero is not a fixed number; it is a dynamic concept, which changes given different clinical scenarios. The fact that there is edema formation and interstitial cell movement following a burn injury suggests that the biological zero should be assessed and subtracted with every flow measurement, such as recommended by Kernick et al.<sup>21</sup>

In a series of patients scanned every 4 hours during the first 48 hours of resuscitation, Jaskille and co-workers<sup>35,36</sup> noted that the measured PU (in non-burned skin) did not follow a linear pattern, rather there were peaks and valleys, which corresponded clinically to changes in base deficit and wound pH. The significance of this is that particles other than red blood cells within the capillaries have a measurable

effect on the measured PU. The implication, thus, is that the timing at which the readings are obtained is very important and could have an effect on how reliably they could predict healing. Mileski et al<sup>37</sup> and Riordan et al,<sup>38</sup> in independent studies, found that accuracy of prediction increases with serial or sequential scans over a period of time, rather than relying on a single scan.

Finally, another very important aspect of the laser Doppler imager is the output measurement of PU. Several researchers have given guidelines as to what wounds are expected to heal based on the PU obtained from the scan. These numbers vary widely. Early work using 4-point LD flowmetry suggested a scale between 0 and 1000 and stated that a cutoff point of 80 PU marks the determination of going to heal vs not going to heal,<sup>37</sup> whereas others have established this cutoff at 250 PU.<sup>12</sup> Some researchers have focused the attention on the depth of the wound, a different outcome altogether, and stated that 150 PU signifies a full-thickness wound, using this as the cutoff for the determination that these wounds are not expected to heal,<sup>14,30</sup> while other researchers did not use PU as the output measure-

ment, but rather volts.<sup>10</sup> Finally, there are some that have used a scale between 0 and 256 and have not mentioned what numerical value was used to mark the determination of healing vs not healing, referring simply to high-flow and low-flow areas.<sup>9,11</sup> The fact that different output measurements and scales are used makes comparisons between studies virtually impossible.

One important point that arises from the studies that used the same output measurement and the same scale is the fact that they provide different numbers for those wounds expected and not expected to heal. Not mentioned in any of those studies is the fact that different areas in the body have a different perfusion and what is the potential effect of this baseline differential perfusion on the PU obtained after a burn. In a study of normal volunteers, Allely et al<sup>39</sup> found that the PU in different areas in the face vary widely from a mean of 280 PU in the forehead to a mean of 525 in the nose. What effect, if any, this difference can play in a burn patient is unknown. Furthermore, a word of caution about using measurements on normal volunteers and trying to predict what could happen in burn wounds is derived from the studies of Waxman et al<sup>28</sup>

**Table 1.** Summary of advantages and disadvantages of burn wound assessment tools

Technique	Advantages	Disadvantages
Radioactive isotopes	Radioactive phosphorus ( <sup>32</sup> P) taken up by the skin	Invasive, too cumbersome, poorly reproducible
Nonfluorescent dyes	Differentiate necrotic from living tissue on the surface	No determination of depth of necrosis; many dyes not approved for clinical use
Fluorescent dyes	Approved for clinical use	Invasive; marks necrosis at a fixed distance in millimeters, not accounting for thickness of the skin; large variability
Thermography	Noninvasive, fast assessment	Many false positives and false negatives based on evaporative cooling and presence of blisters; each center needs to validate its own values
Photometry	Portable, noninvasive, fast assessment, validated against senior burn surgeons, and color palette was developed	Single institution experience; expensive?
Liquid crystal film	Inexpensive	Contact with tissue required, unreliable readings
Nuclear magnetic resonance	Water content in tissue differentiates partial- from full-thickness wounds	In vitro assessment only, expensive, time consuming
Nuclear imaging	<sup>99</sup> mTc shows areas of deeper injury	Expensive, very time consuming, not readily available, and invasive
Pulse-echo ultrasound	Noninvasive, easily available	Underestimates depth of injury, operator dependent, and requires contact with tissue
Doppler ultrasound	Noncontact technology available, provides morphologic and flow information	Operator dependent, not as reliable as laser Doppler
Laser Doppler imaging	Noninvasive and noncontact technology, fast assessment, large body of experience in multiple centers, and very accurate prediction in small wounds in stable patients	Readings affected by temperature, distance from wound, wound humidity, angle of recordings, extent of tissue edema, and presence of shock; different versions of the technology available make extrapolation of results difficult

and Barachini et al<sup>29</sup> on the effects of temperature. In their studies, open wounds and healed wounds had different reactions to changes in temperature, so, an extrapolation cannot be reliably performed.

## DISCUSSION

The prediction of which burn wounds are likely to heal is one of the most important and difficult tasks facing the burn surgeon. A variety of techniques have evolved over the past 70 years to aid in this determination, ranging from the injection of radioactive isotopes and vital dyes to the use of thermography, photometry, nuclear imaging, and ultrasound.<sup>7</sup> One of the more recent techniques, and perhaps the most studied, is LDI. Combining laser technology with the Doppler principle, it aims to provide an estimation of the burn wound perfusion, using this as a predictor of healing.

Many authors have suggested that the technique has a very high positive- and negative-predictive value<sup>10,11</sup> and that it can provide an accurate estimate of healing up to 48 hours earlier than clinical judgment.<sup>14</sup> Most of the studies to date, however, have looked at a specific patient population, and many have had a very limited number of subjects (less than 20 subjects in most studies), making broad conclusions difficult. Similarly, some of the limitations of the technique have not been directly discussed. Another difficulty in trying to draw conclusions from the current literature is that most clinicians have used a different methodology, such as using different makes of the machine, different scanning distances, and scanning different body areas, which makes extrapolation between studies virtually impossible. The first step in addressing some of these problems is to understand the technology. Only after a thorough understanding of the science behind the technology, and its limitations, can a more systematic study be undertaken.

Different tissues in the body have a different thickness; similarly, the skin thickness will vary across individuals. These factors are not accounted for by the currently available LD scanners, and this contributes to the lack of uniform, absolute units. Similarly, several other factors affect the measurement, such as the subject's movement, the wound temperature and moisture, the incident angle of the laser, the presence or absence of shock, the extent of tissue edema, and whether the scan is being performed directly on the tissue or through a transparent dressing. This lack of uniformity makes providing guidelines difficult.

Some of these drawbacks notwithstanding, LD scanning has circumvented some of the pitfalls of previous techniques<sup>7</sup> (Table 1). It is not as cumbersome,

more reliable than the injection of radioactive isotopes, provides a more objective measurement, is less invasive than the injection of vital dyes, and is less operator-dependant than pulse-echo and Doppler ultrasound. No comparative study has been performed between the different adjuvant techniques, and a comparative study between LD scanning with some of the newer thermography techniques, such as active dynamic thermography<sup>40</sup> or infrared thermography<sup>41</sup> would provide an interesting discussion.

Although more uniform and systematic research is needed, LD has brought technology closer to provide a reliable adjuvant to the clinical prediction of healing. The final answer probably lies in a tool, which combines different techniques.

## REFERENCES

1. Moritz AR. Studies of thermal injury: III. The pathology and pathogenesis of cutaneous burns. An experimental study. *Am J Pathol* 1947;23:915.
2. Jackson DM. The diagnosis of the depth of burning. *Br J Surg* 1949;40:588.
3. Janzekovic Z. A new concept in the early excision and immediate grafting of burns. *J Trauma* 1970;10:1103-8.
4. Hlava P, Moserova J, Konigova R. Validity of clinical assessment of the depth of a thermal injury. *Acta Chir Plast* 1983; 25:202-8.
5. Heimbach DM, Afromowitz MA, Engrav LH, Marvin JA, Perry B. Burn depth estimation—man or machine. *J Trauma* 1984;24:373-8.
6. Brown RF, Rice P, Bennett NJ. The use of laser Doppler imaging as an aid in clinical management decision making in the treatment of vesicant burns. *Burns* 1998;24: 692-8.
7. Jaskille AD, Shupp JW, Jordan MH, et al. Critical review of burn depth assessment techniques: Part I. Historical review. *J Burn Care Res* 2009;30:937-47.
8. Stern MD. In vivo evaluation of microcirculation by coherent light scattering. *Nature* 1975;254:56-8.
9. Niazi ZB, Essex TJ, Papini R, Scott D, McLean NR, Black MJ. New laser Doppler scanner, a valuable adjunct in burn depth assessment. *Burns* 1993;19:485-9.
10. Kloppenberg FW, Beerthuisen GI, ten Duis HJ. Perfusion of burn wounds assessed by laser doppler imaging is related to burn depth and healing time. *Burns* 2001;27:359-63.
11. Pape SA, Skouras CA, Byrne PO. An audit of the use of laser Doppler imaging (LDI) in the assessment of burns of intermediate depth. *Burns* 2001;27:233-9.
12. La Hei ER, Holland AJ, Martin HC. Laser Doppler imaging of paediatric burns: burn wound outcome can be predicted independent of clinical examination. *Burns* 2006; 32:550-3.
13. Baker RD, Weinand C, Jeng JC, et al. Using ordinal logistic regression to evaluate the performance of laser-Doppler predictions of burn-healing time. *BMC Med Res Methodol* 2009;9:11.
14. Jeng JC, Bridgeman A, Shivan L, et al. Laser Doppler imaging determines need for excision and grafting in advance of clinical judgment: a prospective blinded trial. *Burns* 2003;29: 665-70.
15. Chatterjee JS. A critical evaluation of the clinimetrics of laser Doppler as a method of burn assessment in clinical practice. *J Burn Care Res* 2006;27:123-30.
16. Briers JD. Laser Doppler, speckle and related techniques for

- blood perfusion mapping and imaging. *Physiol Meas* 2001; 22:R35–66.
17. Murray AK, Gorodkin RE, Moore TL, Gush RJ, Herrick AL, King TA. Comparison of red and green laser doppler imaging of blood flow. *Lasers Surg Med* 2004;35:191–200.
  18. Bray R, Forrester K, Leonard C, McArthur R, Tulip J, Lindsay R. Laser Doppler imaging of burn scars: a comparison of wavelength and scanning methods. *Burns* 2003;29:199–206.
  19. Morales F, Graaff R, Smit AJ, Gush R, Rakhorst G. The influence of probe fiber distance on laser Doppler perfusion monitoring measurements. *Microcirculation* 2003;10:433–41.
  20. Tenland T, Salerud EG, Nilsson GE, Oberg PA. Spatial and temporal variations in human skin blood flow. *Int J Microcirc Clin Exp* 1983;2:81–90.
  21. Kernick DP, Tooke JE, Shore AC. The biological zero signal in laser Doppler fluximetry—origins and practical implications. *Pflügers Arch* 1999;437:624–31.
  22. Zhong J, Nilsson GE, Salerud GE, Seifalian AM. A note on the compartmental analysis and related issues in laser Doppler flowmetry. *IEEE Trans Biomed Eng* 1998;45:534–7.
  23. Zhong J, Seifalian AM, Salerud GE, et al. A mathematical analysis on the biological zero problem in laser Doppler flowmetry. *IEEE Trans Biomed Eng* 1998;45:354–64.
  24. Petersen LJ, Kristensen JK. Simultaneous assessment of blood flow in UVB-inflamed human skin by laser Doppler flowmetry and the 133-xenon washout technique. *Acta Derm Venereol* 1991;71:461–4.
  25. Wahlberg E, Olofsson P, Swedenborg J, Fagrell B. Effects of local hyperemia and edema on the biological zero in laser Doppler fluxmetry (LD). *Int J Microcirc Clin Exp* 1992;11:157–65.
  26. Essex TJ, Byrne PO. A laser Doppler scanner for imaging blood flow in skin. *J Biomed Eng* 1991;13:189–94.
  27. Briers JD, Richards G, He XW. Capillary blood flow monitoring using speckle based contrast analysis (LASCA). *J Biomed Opt* 1999;4:164–75.
  28. Waxman K, Lefcourt N, Achauer B. Heated laser Doppler flow measurements to determine depth of burn injury. *Am J Surg* 1989;157:541–3.
  29. Barachini P, Vezzoni GM, Palombo C, Franzoni F, Bigalli G. Skin blood flow pattern in burns outcomes. *Burns* 2004;30:312–6.
  30. McGill DJ, Sorensen K, MacKay IR, Taggart I, Watson SB. Assessment of burn depth: a prospective, blinded comparison of laser Doppler imaging and videomicroscopy. *Burns* 2007; 33:833–42.
  31. Kernick DP, Shore AC. Characteristics of laser Doppler perfusion imaging in vitro and in vivo. *Physiol Meas* 2000;21: 333–40.
  32. Droog EJ, Steenbergen W, Sjöberg F. Measurement of depth of burns by laser Doppler perfusion imaging. *Burns* 2001;27: 561–8.
  33. Svedman C, Cherry GW, Strigini E, Ryan TJ. Laser Doppler imaging of skin microcirculation. *Acta Derm Venereol* 1998; 78:114–8.
  34. Holland AJ, Ward D, Farrell B. The influence of burn wound dressings on laser Doppler imaging assessment of a standardized cutaneous injury model. *J Burn Care Res* 2007;28: 871–8.
  35. Jaskille AD, Jeng JC, Sokolich JC, Lunsford P, Jordan MH. Repetitive ischemia-reperfusion injury: a plausible mechanism for documented clinical burn-depth progression after thermal injury. *J Burn Care Res* 2007;28:13–20.
  36. Jeng JC, Jaskille AD, Lunsford PM, Jordan MH. Improved markers for burn wound perfusion in the severely burned patient: the role for tissue and gastric Pco<sub>2</sub>. *J Burn Care Res* 2008;29:49–55.
  37. Mileski WJ, Atilas L, Purdue G, et al. Serial measurements increase the accuracy of laser Doppler assessment of burn wounds. *J Burn Care Rehabil* 2003;24:187–91.
  38. Riordan CL, McDonough M, Davidson JM, et al. Noncontact laser Doppler imaging in burn depth analysis of the extremities. *J Burn Care Rehabil* 2003;24:177–86.
  39. Allely RR, Van-Buendia LB, Jeng JC, et al. Laser Doppler imaging of cutaneous blood flow through transparent face masks: a necessary preamble to computer-controlled rapid prototyping fabrication with submillimeter precision. *J Burn Care Res* 2008;29:42–8.
  40. Renkielska A, Nowakowski A, Kaczmarek M, Ruminski J. Burn depths evaluation based on active dynamic IR thermal imaging—a preliminary study. *Burns* 2006;32: 867–75.
  41. Saxena AK, Willital GH. Infrared thermography: experience from a decade of pediatric imaging. *Eur J Pediatr* 2008;167: 757–64.