

Novel Application of a Spatial Frequency Domain Imaging System to Determine Signature Spectral Differences Between Infected and Noninfected Burn Wounds

Thu T. A. Nguyen, MS,* Jessica C. Ramella-Roman, PhD,†
Lauren T. Moffatt, PhD,‡ Rachel T. Ortiz, MS,‡ Marion H. Jordan, MD, FACS,‡
Jeffrey W. Shupp, MD†‡

Complications of infection can increase burn-related morbidity and mortality. Early detection of burn wound infection could lead to more precise and effective treatment, reducing systemic complications and the need for long-term, broad-spectrum intravenous antibiotics. Quantitative cultures from biopsies are the accepted standard to determine infection. However, this methodology can take days to yield results and is invasive. This investigation focuses on the use of noninvasive imaging to determine the infection status of burn wounds in a controlled in vivo model. Full-thickness burn wounds were created on the dorsum of adult male rats ($n = 6$). Twenty-four hours after burn wound creation, wounds in the “Infected” group were inoculated with a vehicle containing 1×10^8 colony forming unit *Staphylococcus aureus*. “Control” group animals received vehicle alone. Subsequently, the wounds were imaged daily for a total of 10 days and the differences of skin optical properties were assessed using spatial frequency domain imaging at 16 different wavelengths from 500 to 700 nm. Regions of interest on the resulting images were selected and averaged at each time point. Statistically significant differences in average absorption and reduced scattering coefficients (μ_a and μ_s) at 620 and 700 nm were observed between the two groups ($P < .05$). Differential optical properties were most evident by day 4 and persisted throughout the time course. Differential signature changes in optical properties are evident in infected burn wounds. This novel application of spatial frequency domain imaging may prove to be a valuable adjunct to burn wound assessment. Further work will be aimed at determining dose-response relationships and prokaryotic species differences. (*J Burn Care Res* 2013;34:44–50)

Complications resulting from infection in burn patients can cause drastic increases in morbidity and mortality.^{1,2} Local and systemic impacts may result from burn wound infections, including delayed healing, immune reactions, and shock.³ Early intervention including bacteriostatic and

bacteriocidal topical and systemic treatments can reduce these risks; however, antibiotic treatment regimens must be carefully considered and chosen according to pathogen characteristics. Treating a bacterial infection at an inappropriate time or with a drug with a mode of action that is not suited for the pathogen can be detrimental and potentially result in a worse outcome than not treating at all.⁴ Early diagnosis of pathogen presence and traits would allow for more tailored, appropriate antibiotic treatment regimens; however, limitations exist in diagnostics available for determining burn wound infection status and type.

Currently, clinicians rely on quantitative cultures of wounds or blood, which involve swabs, biopsies, or blood draws. These methods are invasive and not

*From the Departments of *Electrical Engineering and †Biomedical Engineering, School of Engineering, The Catholic University of America; and ‡Department of Surgery, The Burn Center, MedStar Washington Hospital Center, MedStar Health Research Institute, Washington, DC.*

Address correspondence to Jeffrey W. Shupp, MD, 110 Irving Street, NW, Suite 3B-55, Washington, DC 20010.

*Copyright © 2013 by the American Burn Association
1559-047X/2013*

DOI: 10.1097/BCR.0b013e318269be30

ideal, as they can increase the trauma to the wound and cause discomfort for the patient. Furthermore, cultures may take 2 to 3 days to yield definitive results, allowing additional time for the pathogens to invade the host system.

Spatial frequency domain imaging (SFDI) is a novel, noninvasive imaging technique used to calculate the quantitative optical properties, absorption coefficient μ_a , and reduced scattering coefficient μ_s , of a biological tissue. This technique was first successfully used by Cuccia et al.⁵ The goal of this study was to test the hypothesis that by applying this method to imaging infected and noninfected burn wounds in a controlled model system, infection status based on optical properties could be determined, thereby demonstrating a novel, noninvasive technique for assessing wound infections.

METHODS

Burn Wound Infection Model

The MedStar Health Research Institute Institutional Animal Care and Use Committee reviewed and approved all described animal research. Animals were received and husbandry was provided according to facility standard operating procedures. Six male Sprague Dawley rats (Harlan Labs, Frederick, MD) were anesthetized and prepared as described previously.⁶

Burn wounds were created on the dorsum of all animals, as described by Shupp et al.⁶ Briefly, custom-milled aluminum branding irons with 2×2 cm base areas were heated to 100°C . Irons were applied to the prepared skin for 12 seconds, using only the weight of the iron and no additional pressure, to create two paired wounds, each 1 cm away from the spine. Approximately 24 hours after burn wound creation, three animals received an inoculation, as described,⁶ with $200 \mu\text{l}$ of a vehicle containing 1×10^8 colony forming unit (CFU) methicillin-resistant *Staphylococcus aureus* to both wounds, whereas the wounds of the remaining three animals were treated with culture broth alone (sham).

Experimental Design

Twenty-four hours after inoculation, animals were anesthetized, weighed, placed on a warming blanket, and monitored, and their right dorsal wound imaged using SFDI. These assessments under anesthesia were repeated daily for 9 more days. Biopsies (2 mm punch) were also taken for quantitative wound cultures from the left wound of each animal on days 0, 2, 5, 7, and 10, to preserve the right wound for imaging only.

Quantitative Cultures

Biopsies were weighed and homogenized in sterile saline using a LabGen Homogenizer (Omni International, Kennesaw, GA) with disposable, sterilized plastic probes. The homogenates were then serially diluted in sterile saline, with $100 \mu\text{l}$ of each dilution plated on Mannitol Salt Agar plates (BD, Franklin Lakes, NJ), selective for *S. aureus*. Plates were incubated at 37°C until colony counts were performed 24 and 48 hours after plating. Counts (positive, yellow colonies only) were then used to calculate colony forming units per gram (CFU/g) for each biopsy. This method is described in Shupp et al.⁶ Means (CFU/g) were then calculated for wounds from infected animals ($n = 3$) and noninfected animals ($n = 3$) for each time point.

Spatial Frequency Domain Imaging

An SFDI system was built to image infected and noninfected burn wounds daily in a 10-day set. Imaging was conducted at 16 different wavelengths from 500 to 700 nm. SFDI images were postprocessed to calculate optical properties calculations that were then related to pathophysiology of the wounds. Differences of optical properties between two groups (infected and noninfected wounds) were assessed. The SFDI system was connected to a laser Doppler imaging (LDI) tool and constituted an integrated system as shown in Figure 1A, 1B. The LDI system was used to measure blood perfusion in wounds of two groups of animals. The LDI results were then used, combined with SFDI results, to obtain a better understanding of pathophysiological changes in the wounds. In this study, results of LDI are not shown.

Samples

In the system, a light source is modulated to project sinusoidal fringe patterns on a sample at three different phases (0, $2\pi/3$, $4\pi/3$) of a specific spatial frequency f (per millimeter), and three images of diffuse reflected light from the sample are acquired (Figure 1B). A value of spatial frequency of $f = 0.2/\text{mm}$ was selected to control the optical penetration depth of light into the skin. With this value, light can penetrate into the skin dermal layer (with penetration depth of approximately $700 \mu\text{m}$). The optical properties of the skin are wavelength-dependent; in this work, 16 wavelengths (500, 516, 529, 541, 545, 556, 560, 570, 577, 584, 588, 596, 620, 632, 650, and 700 nm) were used, and a minimization algorithm was used to extrapolate specific metrics of interest from the calculated optical properties.

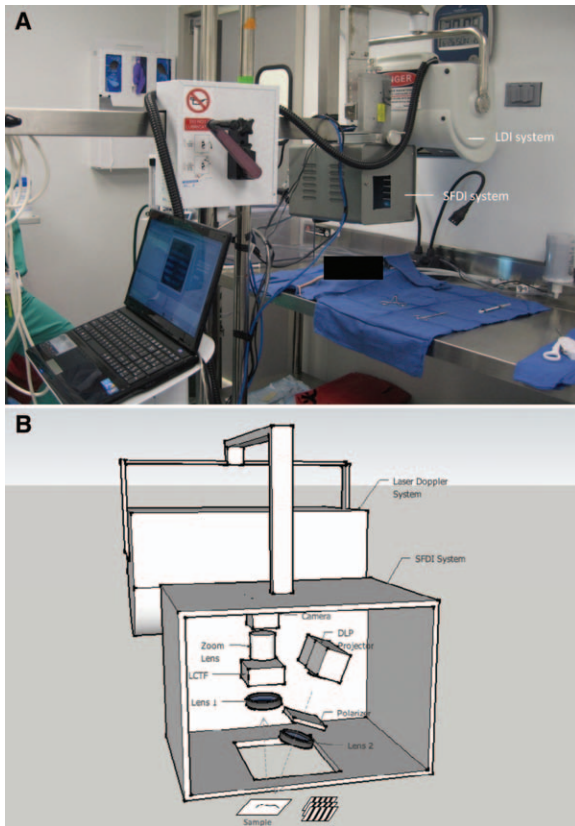


Figure 1. Experimental setup (A) and schematic setup (B) of SFDI and LDI system. *SFDI*, spatial frequency domain imaging; *LDI*, Laser Doppler Imaging; *LCTF*, liquid crystal tunable filter; *DLP*, digital light processing.

Optical Property Analysis

To determine optical properties at one wavelength, three images of the sample were acquired. The diffused reflectance at frequency zero $Rd(0)$ and at frequency f $Rd(f)$ were calculated. These components are the inputs to the Diffusion equation and are ultimately used to calculate μ_a and μ_s . By scanning each pixel of the reflected image, entire two-dimensional maps of μ_a and μ_s can be reconstructed. More details of these calculation steps are described in a previous publication.⁷ The SFDI system was calibrated with polyurethane diffusive phantoms mimicking tissue optical properties.⁸

The achieved μ_a at different wavelengths can be used to determine relative amounts of tissue molecular components. Oxygenated hemoglobin, deoxygenated hemoglobin, melanin concentration, water, and met-hemoglobin are typical metrics of interest. In this study, the maps of absorption coefficients of each wound at desired wavelengths were used to extract a map of oxygen saturation level (SO_2) and a map of blood volume fraction

(HB). A least square fitting method based on the Nelder-Mead simplex minimization algorithm⁹ was applied to Eq. (1)¹⁰ and tabulated values of oxy- and deoxyhemoglobin absorption coefficients μ_{aHB} and μ_{aHB02} ¹⁰ were used to calculate values of SO_2 and HB.

$$\mu_a = B \times [(1 - S) \times \mu_{aHB} + S \times \mu_{aHB02}] + C \quad (1)$$

B represents HB volume fraction, S represents SO_2 , and C is a fixed offset that represents skin background absorption.

In this animal study, the absorption of water and met-hemoglobin are neglected because of their insignificant contribution in comparison with the absorption of the other chromophores (oxy- and deoxyhemoglobin). Nevertheless, the absorption of melanin of rat skin is taken into account. The total absorption of the skin is the summation of the melanin absorption within the epidermal layer and the absorption of oxy- and deoxyhemoglobin within the penetration depth of the light in the dermal layer.

Instrumentation

Our SFDI system included a digital light processing projector (1024×768, maximum contrast 2000:1). Two-dimensional sinusoidal fringe patterns created with MATLAB (Natick, MA) were projected on the skin using a projection lens ($f = 50$ mm). Reflected light from the skin was captured by a monochromatic camera (1024×1024 pixels, CCD Genie Dalsa, Waterloo, Canada) through an imaging zoom lens ($f = 200$ mm, Nikon, Tokyo, Japan). A liquid crystal tunable filter (CRI Inc., Woburn MA) was positioned in front of the camera and was computer controlled, allowing sequential selection of different wavelengths from 400 to 700 nm with a 7 nm bandwidth. A pair of polarizers were assembled on the illumination arm and the receiving arm of our system, and were crossed to each other to avoid skin specular reflection. All components were fixed into a light-tight enclosure. The entire imaging process was set up to run automatically on an area of 3×3 cm on the wounded skin.

RESULTS

Quantitative Cultures

Wound biopsies from animals receiving bacterial inoculation had detectable levels of *S. aureus* growth starting on day 2 (24 hours after inoculation). The mean bacteria load peaked at 6.66×10^{13} CFU/g on day 5, and decreased, but remained at detectable levels until day 10 (Figure 2). Biopsies from animals

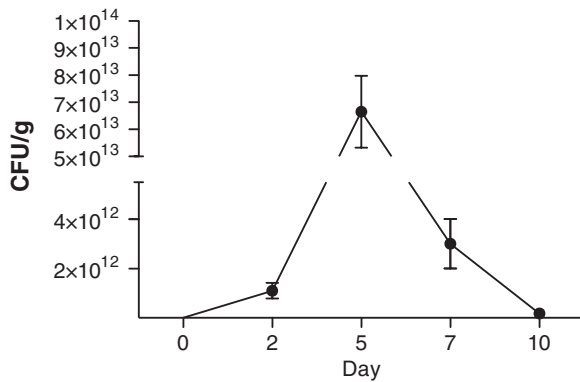


Figure 2. *Staphylococcus aureus* growth in biopsy cultures from infected wounds at five time points. Data shown are means ($n = 3$) with error bars representing SDs. CFU/g, colony forming units/gram.

receiving the sham (media alone) inoculation did not demonstrate a detectable level of *S. aureus* infection at any time point.

Spatial Frequency Domain Imaging

To assess differences between optical properties of the group of infected wounds ($n = 3$) and the group of noninfected wounds ($n = 3$), maps of optical properties (μ_a, μ_s') of each wound were first reconstructed along 16 wavelengths over 12 time points (before burn, immediately after burn, day 1 to day 10). To observe the same skin area throughout the 12 days, regions of interest were selected in correlation with marks created on the skin on the first day using a black permanent marker. Short wavelengths below 620 nm did not penetrate deep enough into the wounds and did not give any helpful information about μ_a and μ_s' . At longer wavelengths (620, 632, 650, and 700 nm), reconstruction results of μ_a of both infected and noninfected wounds indicated an increasing trend along the time course, in most cases. Results of μ_s' of all wounds seemed to increase during the first 2 days postburn, but started decreasing from day 3 and continued in the same trend in the following days. Optical properties changed for all wounds but more significantly for infected wounds. In the imaging wound of one animal, an assumed fungal presence started appearing as white growth on day 5 and drastically scattered light. This infection was not considered in this analysis.

Mean values of absorption coefficients and scattering coefficients on all animals of each group were considered for statistical assessment. For every animal, average values of μ_a and μ_s' of three selected viable regions on the wound were first calculated at each time point and each wavelength, $avg-\mu_a$ and

$avg-\mu_s'$. Figure 3 shows typical reconstruction maps of an infected wound with three selected regions (marked by three squares of white, black, and red color) over 12 time points for absorption coefficient (Figure 3A) and reduced scattering coefficient (Figure 3B) at the wavelength of 700 nm. The color bars on the right hand side in Figure 3A, 3B show the values of absorption coefficient and reduced scattering coefficient maps in the unit of per millimeter.

The mean of three $avg-\mu_a$ values, named $mean-avg-\mu_a$, from three animals in the same group was calculated; a similar procedure was used to obtain a $mean-avg-\mu_s'$. At every wavelength, $mean-avg-\mu_a$ as well as $mean-avg-\mu_s'$ for 12 time points were obtained for the infected group and the noninfected group of animals. Values of SEM of each group were also calculated. A comparison of μ_a and μ_s' values between the two groups of wounds was then conducted by applying a statistical Student *t*-test. The results of absorption coefficient and reduced scattering coefficient showed that there is significant separation ($P < .05$) between the two groups at the observed wavelengths starting at day 4 (Figure 4 and Table 1). SEMs of the two groups are also included. A comparison of mean value of μ_a and μ_s' between the infected group and the noninfected group along the time course (preburn, postburn, day 1 to day 10) is presented in Figure 4 (at wavelength 632 nm) with *P* values listed in Table 1. Similar behavior was noted for 650 and 700 nm data.

The method described above was used to extract fold changes in SO_2 and HB along the time span of the study as shown in Figures 5 and 6. Values of SO_2 and HB of each animal are average values of the three regions of interest previously selected. Figure 5 shows fold changes in mean values of SO_2 level and values of SEM of the two groups at 12 time points. Similarly, Figure 6 shows fold changes in mean values of HB and values of SEMs of the two groups at 12 time points.

DISCUSSION

A nonlethal burn wound infection animal model was successfully investigated during a 10-day time course. SFDI was acquired daily in parallel with LDI and biopsy collection. Optical properties of skin preburn and during 10 days postburn in noninfected and infected wounds were assessed at 16 different wavelengths from 500 to 700 nm. Results at wavelengths above 620 nm clearly showed the expected increase of absorption coefficient of the wounds as well as a decrease in scattering coefficient. Changes

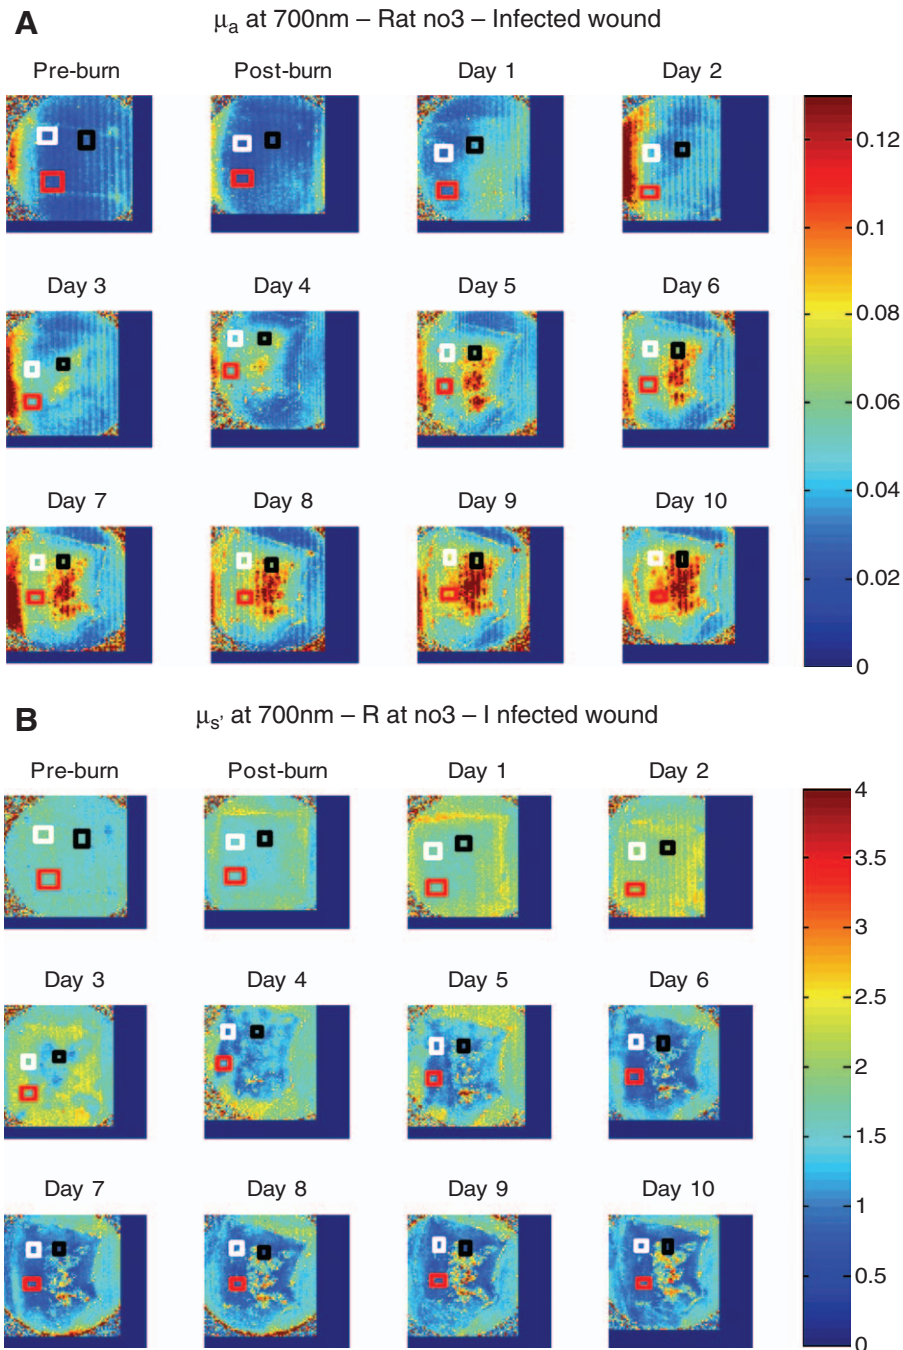


Figure 3. Typical reconstruction maps of an infected wound with three selected regions over 12 time points (before burn, immediately after burn, day 1 to day 10) for absorption coefficient (A) and scattering coefficient (B) at the wavelength of 700 nm.

in infected wounds appeared more dramatically than in noninfected wounds. Statistically significant differences in average absorption and reduced scattering coefficients at 620, 632, 650, and 700 nm were observed between the two groups with $P < .05$.

Blood volume fraction fluctuated in all animals without showing a particular trend for each group, but seemed to increase with both groups

in following the burn event. This result indicates hematocrit increase in the wounds. The change in hematocrit probably resulted from an increase in moving red blood cells, which could be observed in the LDI results. These results (not shown in this article) indicated that blood perfusion of the non-infected group was higher than the infected group from day 4 and kept increasing in the following

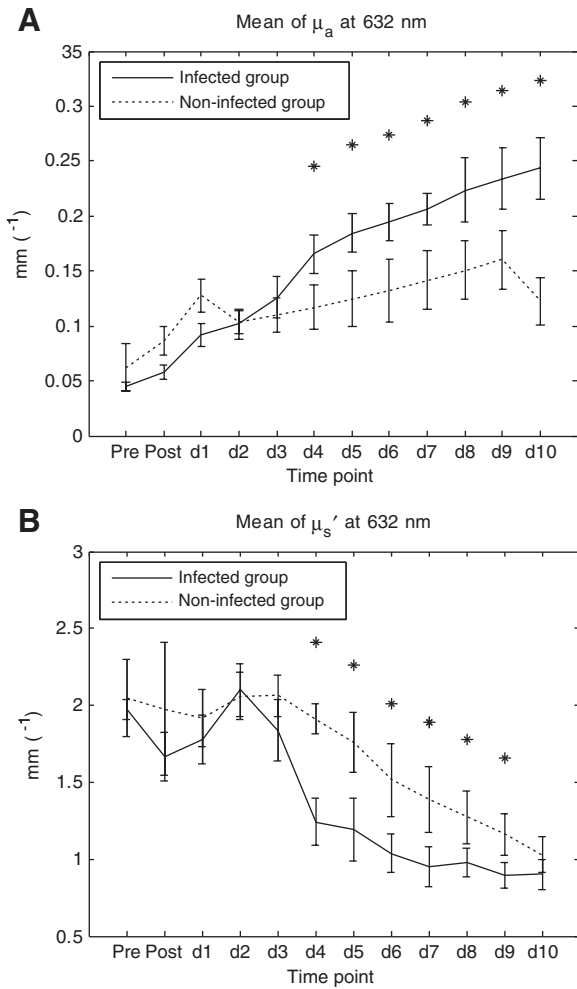


Figure 4. Comparison of mean values of μ_a (A) and μ_s (B) between infected group and noninfected group at wavelength 632 nm. SEMs of the two groups are also included.

days. Higher blood volume fraction as well as blood perfusion appeared in the noninfected wounds compared with infected wounds. Higher oxygen concentration being carried by hemoglobin to the

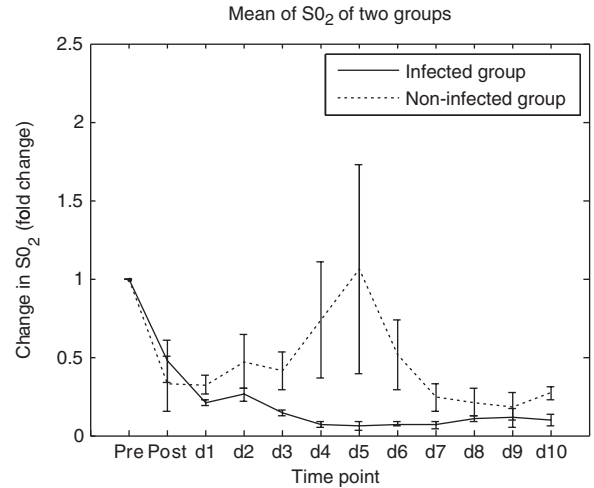


Figure 5. Fold changes in mean values of SO_2 level and values of SEM of the two groups at 12 time points. SO_2 oxygen saturation level.

noninfected wounds may be expected. This was observed in our oxygen saturation results. Calculated mean value of SO_2 increased in the noninfected group, but remained unchanged in the infected group.

All changes in skin properties were most evident by day 4 and persisted throughout the time course. The differential changes that occurred between the two groups indicated a recognizable sign of infection and a possible method to separate noninfected and infected wounds. Results at different wavelengths contained information about different layers in the wounds. Wavelengths shorter than 620 nm were mostly absorbed by the superficial layers of the skin and did not provide useful information. This is probably due to postburn eschar developing in the top layer of the skin.

We believe that the results of our analysis will help in the diagnosis of the infection status of a wound.

Table 1. Probability values of the comparisons of mean value of μ_a and μ_s between infected group and noninfected group at wavelength 620, 632, 650, and 700 nm

		Preburn	Postburn	Day 1	Day 2	Day 3	Day 4	Day 5	Day 6	Day 7	Day 8	Day 9	Day 10
620 nm	μ_a	0.21	0.01	0.02	0.71	0.29	0.02	0.01	0.02	0.01	0.02	0.02	0.00
	μ_s	0.62	0.33	0.26	0.98	0.15	0.00	0.01	0.03	0.02	0.05	0.03	0.25
632 nm	μ_a	0.22	0.00	0.02	0.82	0.40	0.02	0.00	0.01	0.00	0.02	0.02	0.00
	μ_s	0.66	0.27	0.26	0.73	0.07	0.00	0.01	0.02	0.03	0.02	0.01	0.28
650 nm	μ_a	0.34	0.02	0.01	0.80	0.23	0.04	0.01	0.02	0.01	0.02	0.01	0.00
	μ_s	0.45	0.32	0.38	0.71	0.04	0.00	0.01	0.03	0.03	0.02	0.01	0.25
700 nm	μ_a	0.18	0.05	0.00	0.90	0.08	0.10	0.04	0.01	0.00	0.03	0.00	0.00
	μ_s	0.56	0.59	0.39	0.78	0.01	0.00	0.02	0.01	0.01	0.00	0.00	0.34

From day 4, values of $P < .05$ are indicated in boldface.

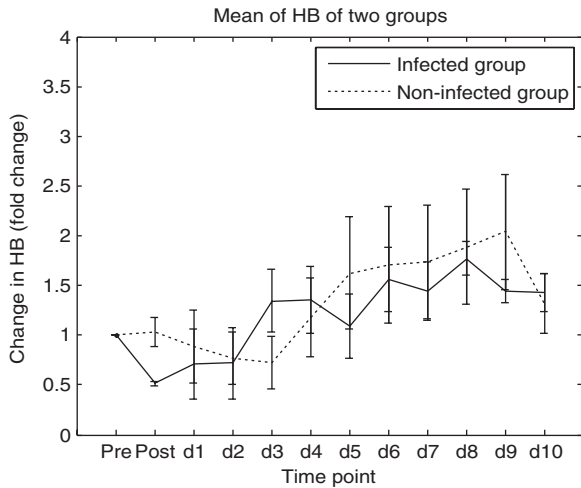


Figure 6. Fold changes in mean values of HB and SEMs of the two groups at 12 time points. *HB*, blood volume fraction.

This novel application of SFDI may prove to be a valuable adjunct to burn wound assessment. Future work with increased sample size will be aimed at determining dose-response relationships and prokaryotic species differences along with in vitro spectral analysis.

REFERENCES

- Shurland S, Zhan M, Bradham DD, Roghmann MC. Comparison of mortality risk associated with bacteremia due to methicillin-resistant and methicillin-susceptible *Staphylococcus aureus*. *Infect Control Hosp Epidemiol* 2007;28:273-9.
- Branski LK, Al-Mousawi A, Rivero H, Jeschke MG, Sanford AP, Herndon DN. Emerging infections in burns. *Surg Infect (Larchmt)* 2009;10:389-97.
- Kaiser ML, Thompson DJ, Malinoski D, Lane C, Cinat ME. Epidemiology and risk factors for hospital-acquired methicillin-resistant *Staphylococcus aureus* among burn patients. *J Burn Care Res* 2011;32:429-34.
- Schlievert PM, Kelly JA. Clindamycin-induced suppression of toxic-shock syndrome-associated exotoxin production. *J Infect Dis* 1984;149:471.
- Cuccia DJ, Bevilacqua F, Durkin AJ, Ayers FR, Tromberg BJ. Quantitation and mapping of tissue optical properties using modulated imaging. *J Biomed Opt* 2009;14:024012.
- Shupp JW, Pavlovich AR, Jeng JC, et al. Epidemiology of bloodstream infections in burn-injured patients: a review of the national burn repository. *J Burn Care Res* 2010;31:521-8.
- Nguyen TTA, Shupp JW, Moffatt LT, Jordan MH, Leto EJ, Ramella-Romen JC. Assessment of the pathophysiology of injured tissue with an in vivo electrical injury model. *IEEE J Quantum Electron* 2012;4:1403-11.
- Moffitt T, Chen YC, Pahl SA. Preparation and characterization of polyurethane optical phantoms. *J Biomed Opt* 2006;11:041103.
- Nelder JA, Mead R. A Simplex Method for Function Minimization. *Comp J* 1965;7:308-13.
- Jacques, SL. Spectroscopic determination of tissue optical properties using optical fiber spectrometer. [Online]; available at <http://omlc.ogi.edu/news/apr08/skinspectra/index.html>.